




# GALAXY GX2 Incident Report

**Incident Type:** Exposure Low Alarm      Gas Type: Carbon Monoxide  
**Incident Date/Time:** 8/24/2014 5:12:00 PM      Timezone: Eastern Standard Time  
**Instrument Type:** ALTAIR Pro      SerialNumber: 4302047  
**Company:**      User: CO  
**Department:**      Date Field: Timestamp Of Event

## Event Graph

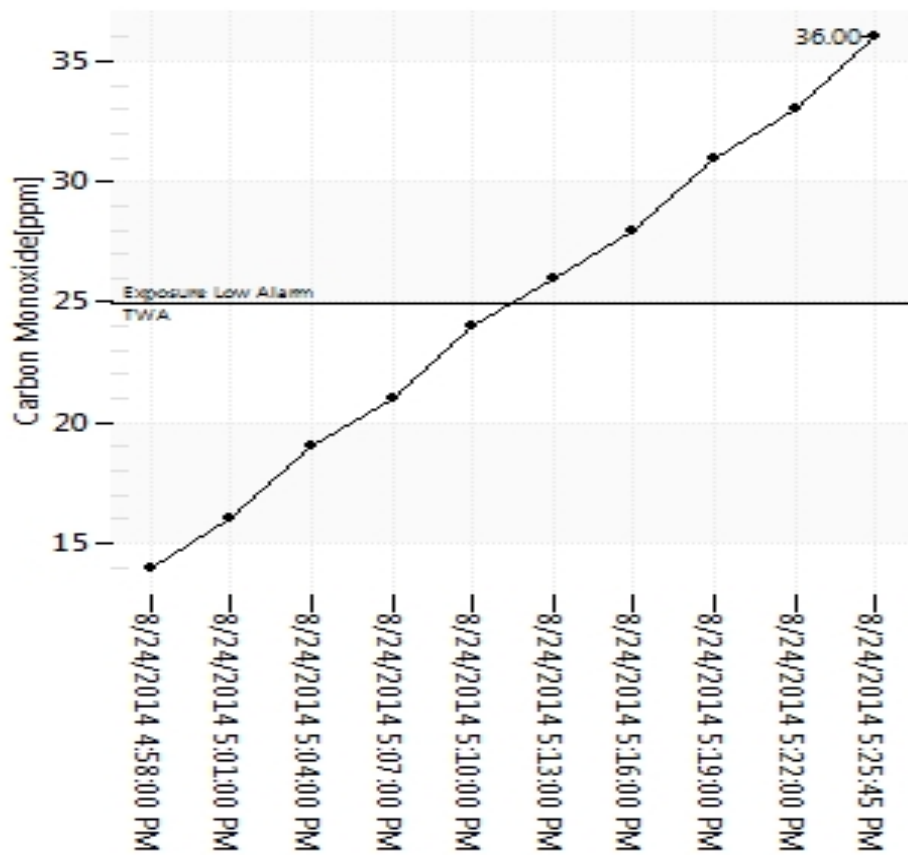

[Carbon Monoxide] Peak Values 14.00 16.00 19.00 21.00 24.00 26.00 28.00 31.00 33.00 36.00

## Calibration Data

Gas	Sensor Enabled	Calibration Result	Expected Value	Found Value
	<input type="checkbox"/>		-	-

## Periodic Data

Carbon Monoxide

Timestamp	Gas	Average Value	Peak Value	Temperature
8/24/2014 4:58:00 PM	Carbon Monoxide	0.00 ppm	14.00 ppm	30.00°C
8/24/2014 5:01:00 PM	Carbon Monoxide	0.00 ppm	16.00 ppm	30.00°C
8/24/2014 5:04:00 PM	Carbon Monoxide	0.00 ppm	19.00 ppm	30.00°C
8/24/2014 5:07:00 PM	Carbon Monoxide	0.00 ppm	21.00 ppm	30.00°C
8/24/2014 5:10:00 PM	Carbon Monoxide	0.00 ppm	24.00 ppm	31.00°C
8/24/2014 5:13:00 PM	Carbon Monoxide	0.00 ppm	26.00 ppm	31.00°C
8/24/2014 5:16:00 PM	Carbon Monoxide	0.00 ppm	28.00 ppm	31.00°C
8/24/2014 5:19:00 PM	Carbon Monoxide	0.00 ppm	31.00 ppm	31.00°C
8/24/2014 5:22:00 PM	Carbon Monoxide	0.00 ppm	33.00 ppm	31.00°C
8/24/2014 5:25:45 PM	Carbon Monoxide	0.00 ppm	36.00 ppm	32.00°C